

*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown *Atty Docket: DEXCOM.037A*

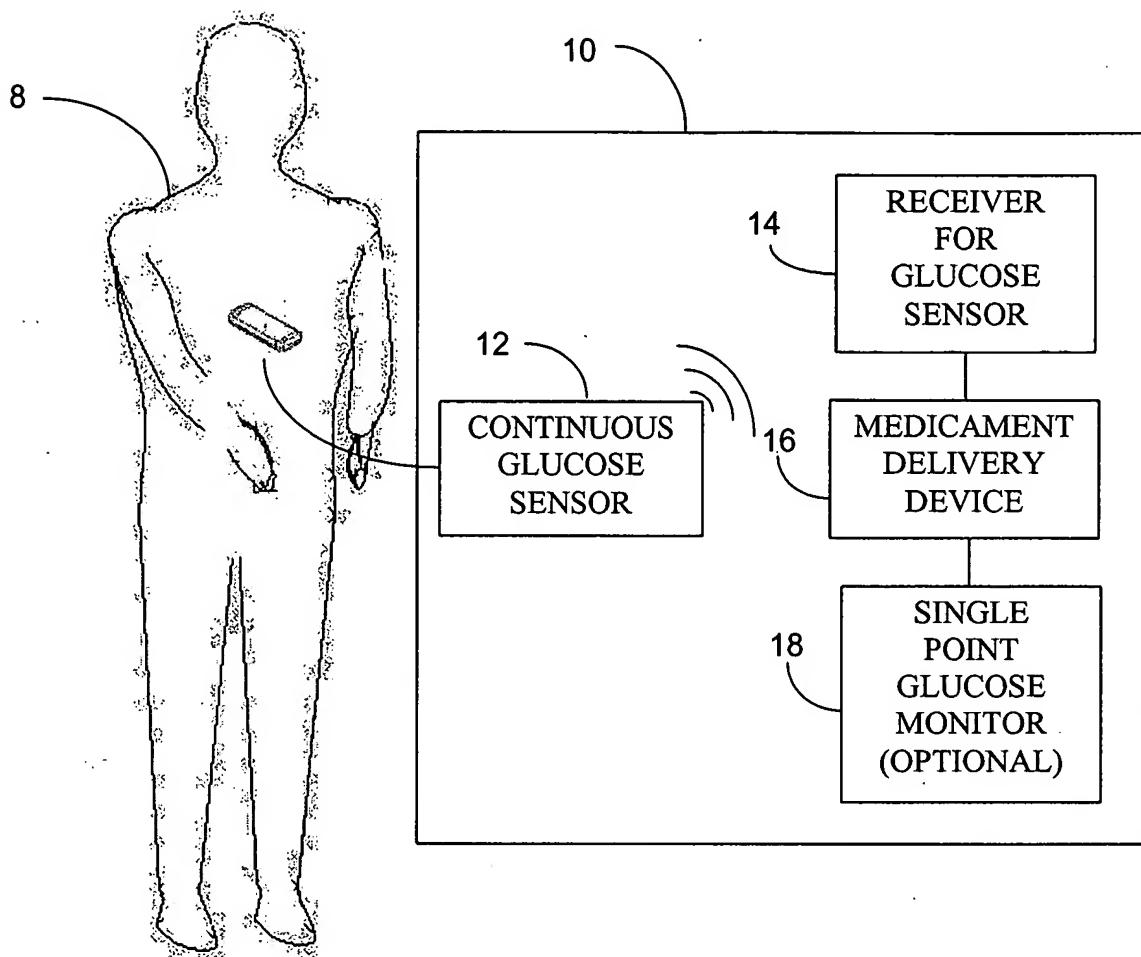


FIG. 1

*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown Atty Docket: DEXCOM.037A

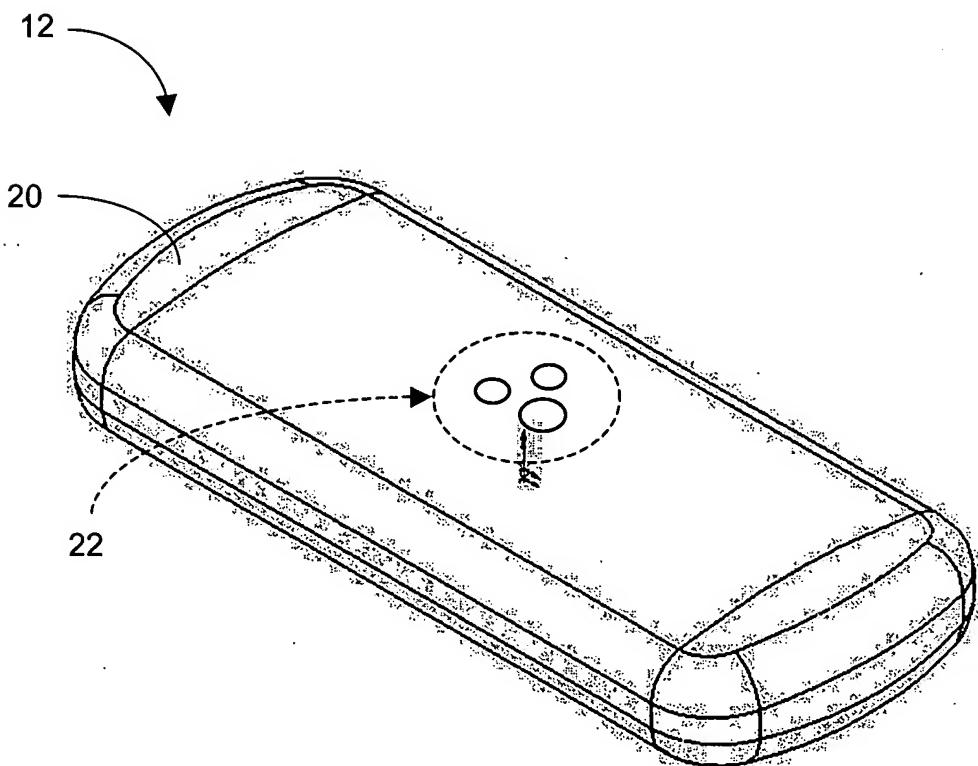


FIG. 2

*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown *Atty Docket: DEXCOM.037A*






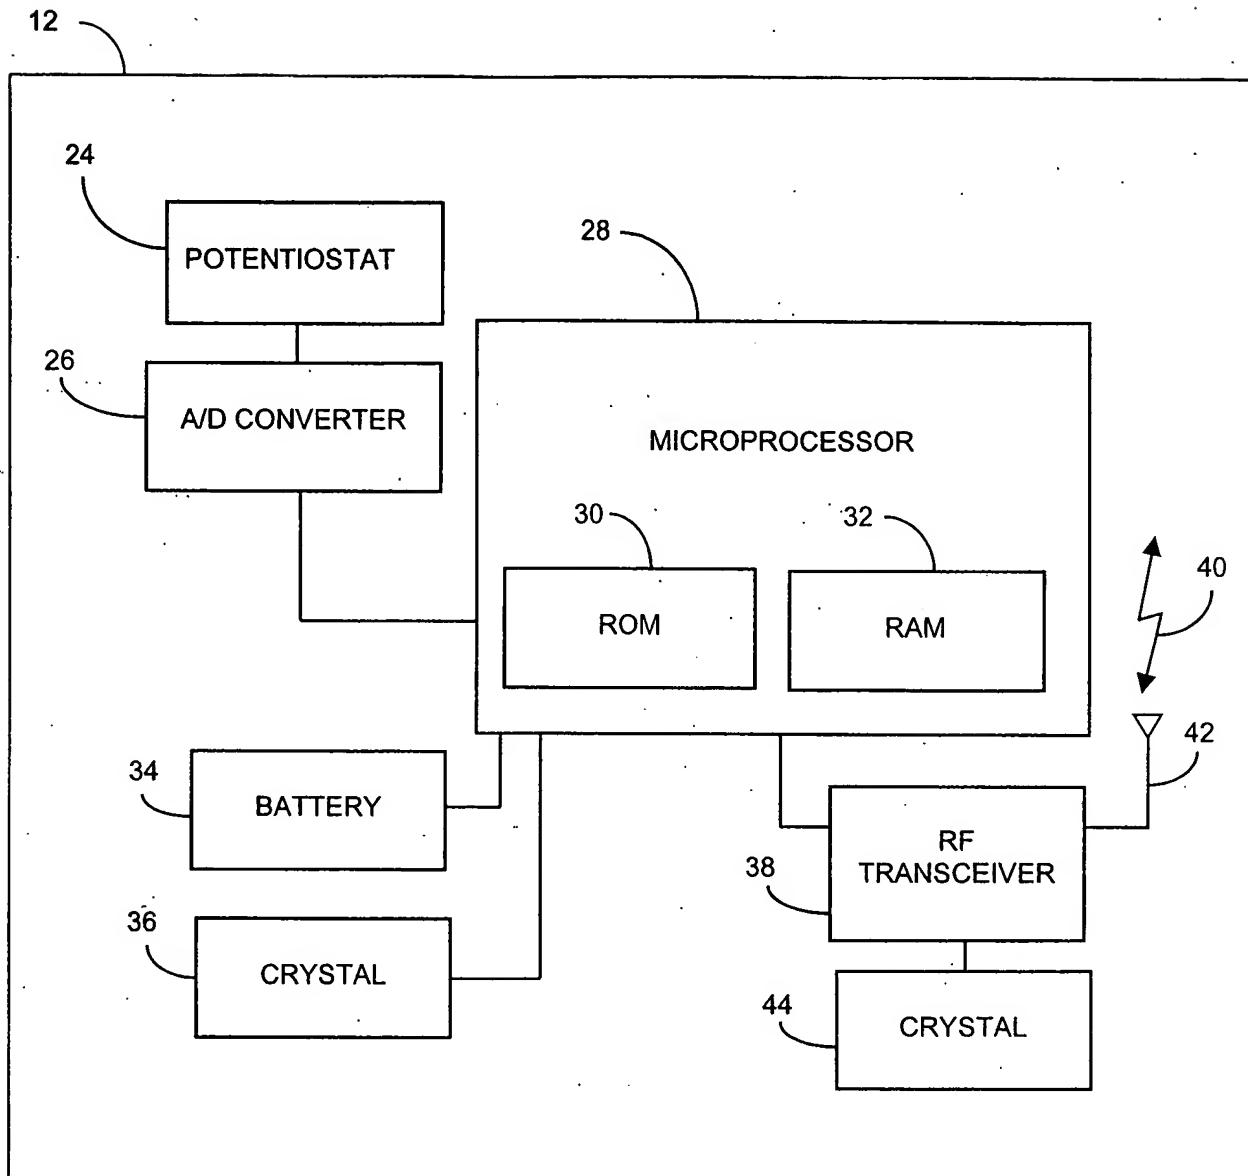


FIG. 3



*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown *Atty Docket: DEXCOM.037A*

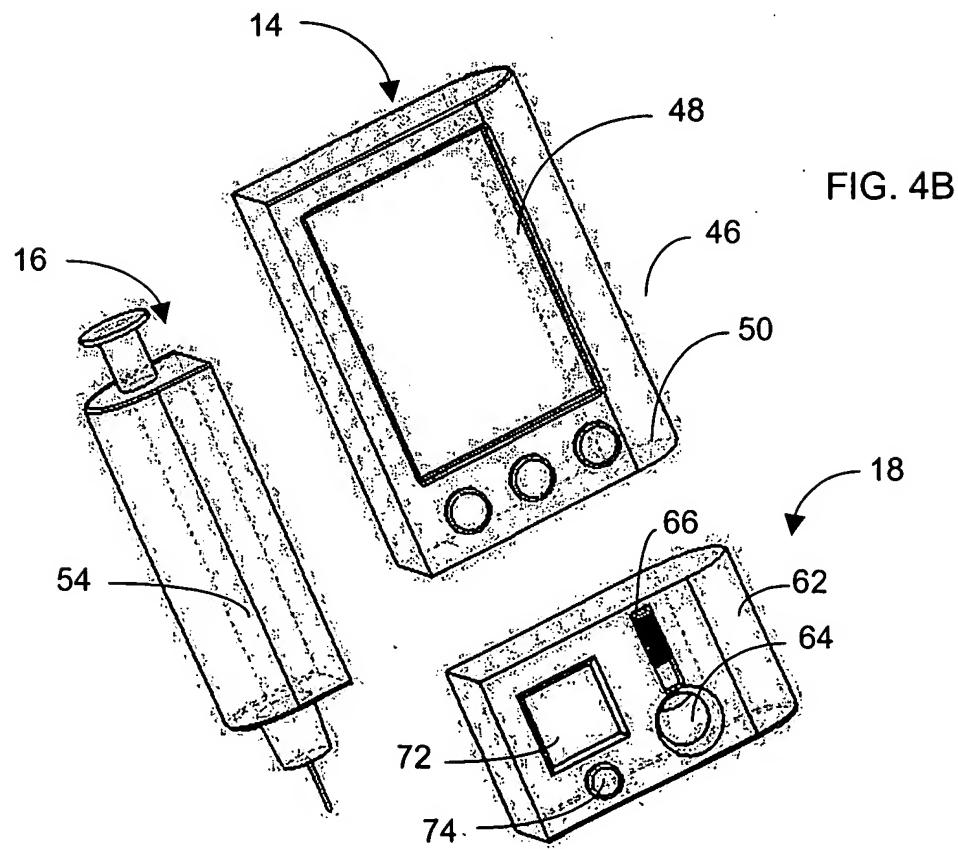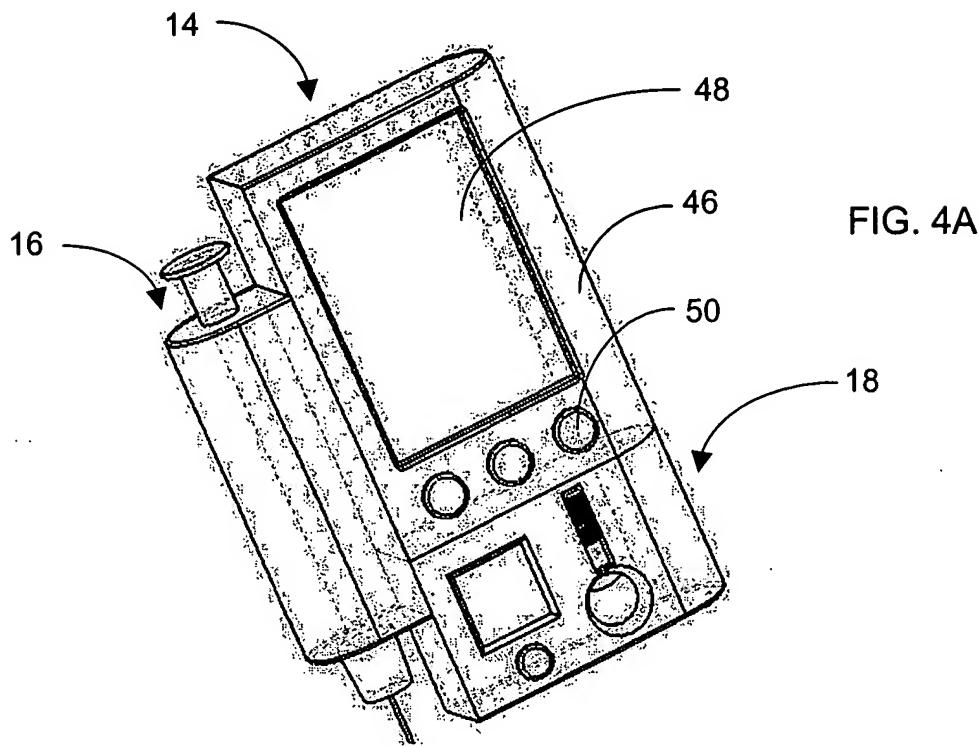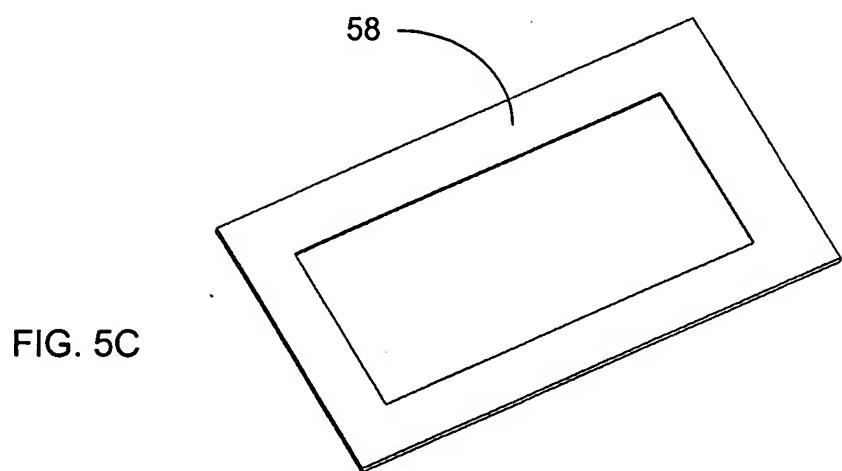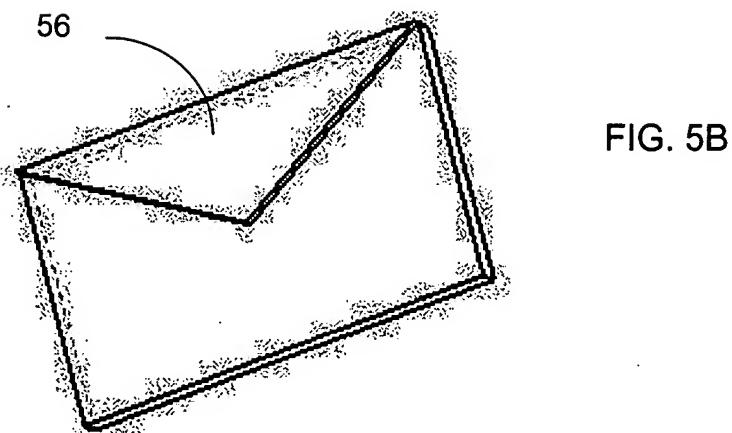

*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown *Atty Docket: DEXCOM.037A*

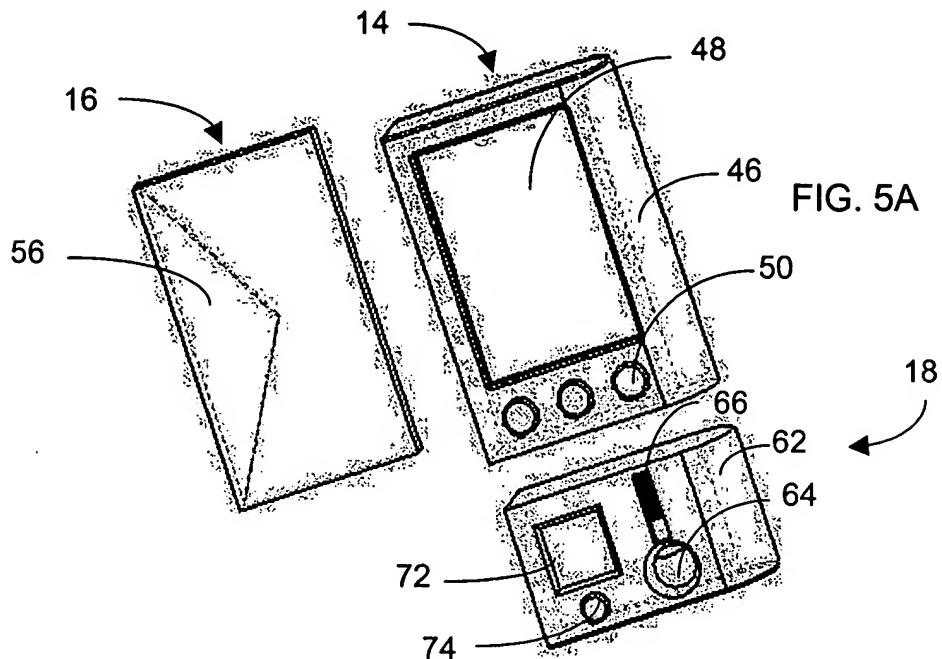

*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown *Atty Docket: DEXCOM.037A*

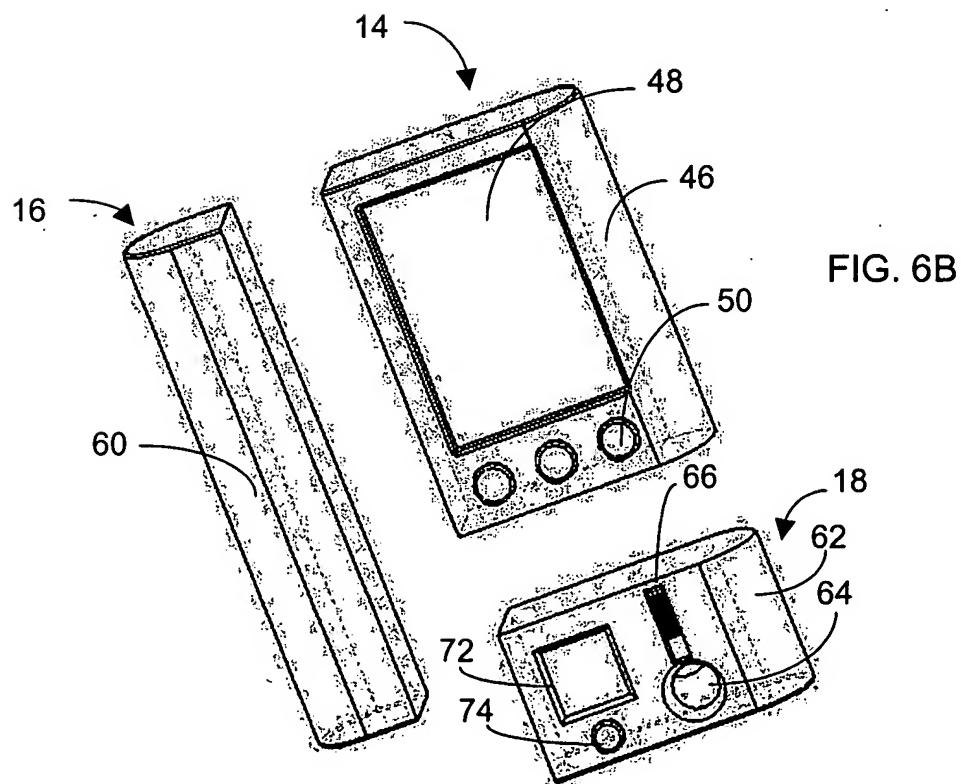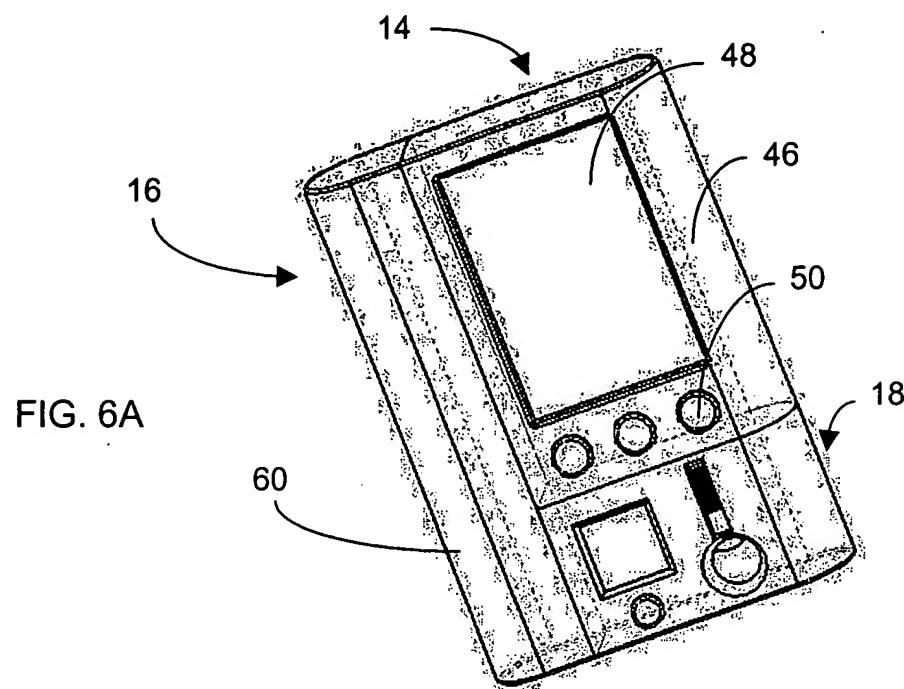

*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown *Atty Docket: DEXCOM.037A*

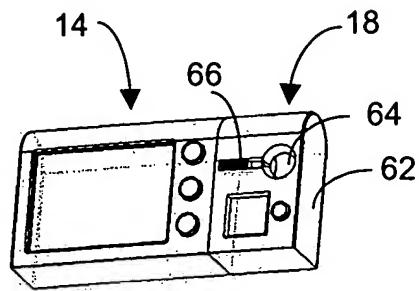
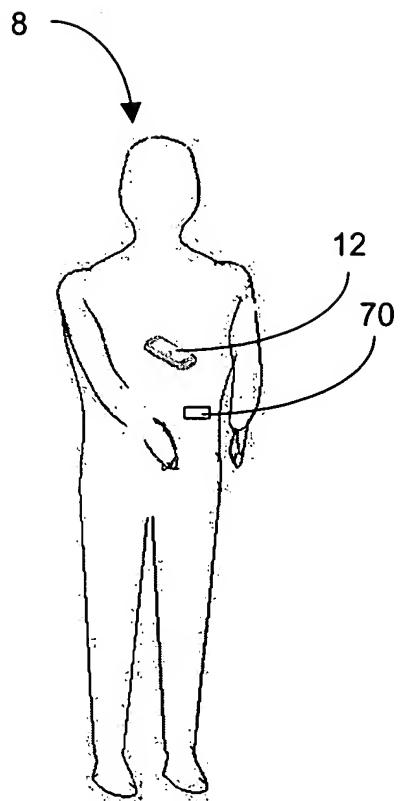


FIG. 7B

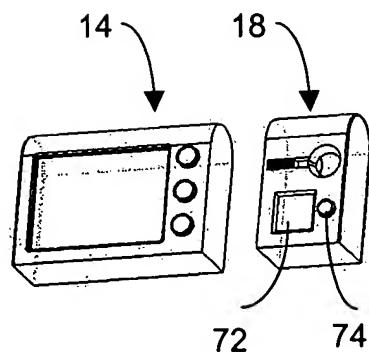


FIG. 7A

FIG. 7C

*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown *Atty Docket: DEXCOM.037A*

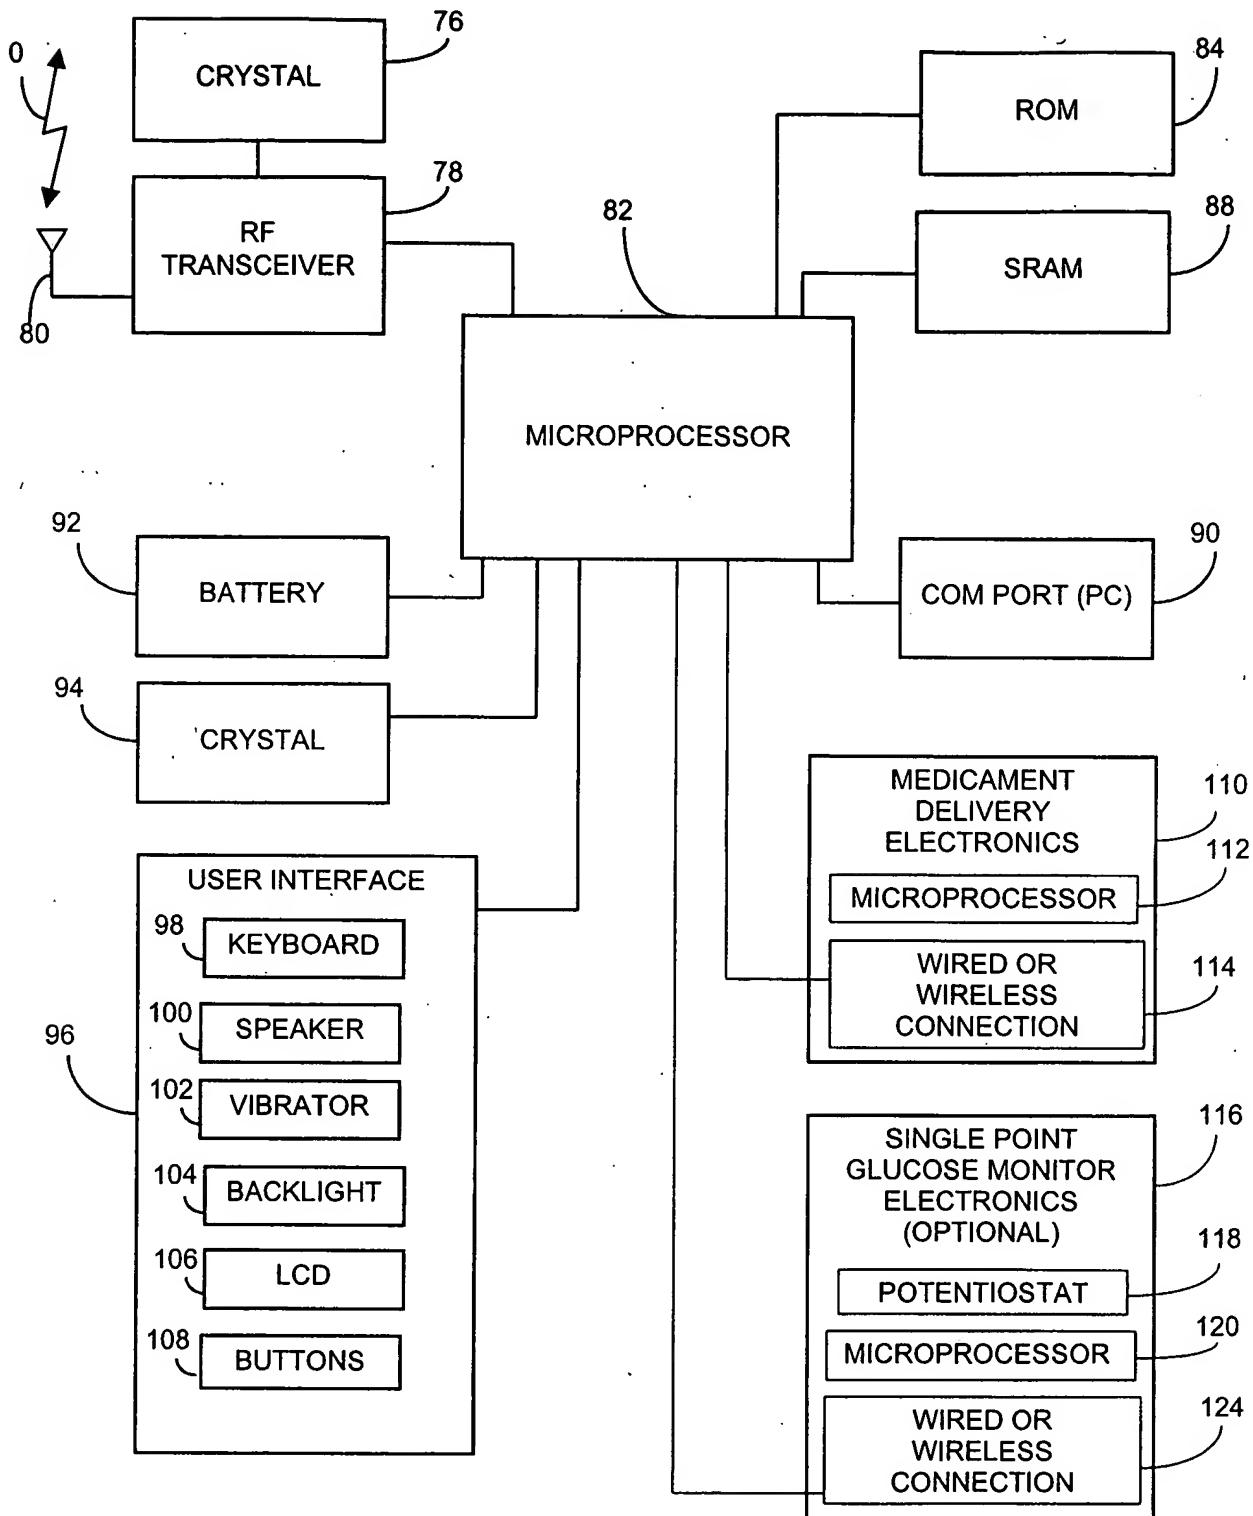


FIG. 8

*INTEGRATED DELIVERY DEVICE FOR CONTINUOUS GLUCOSE
SENSOR*
Brauker, et al.
Appl. No.: Unknown Atty Docket: DEXCOM.037A

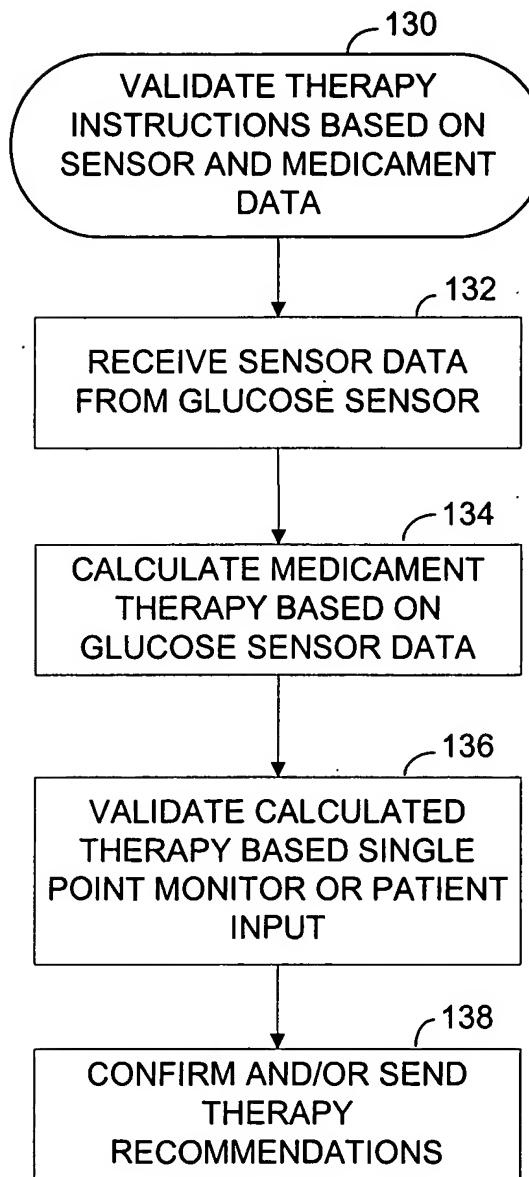


FIG. 9

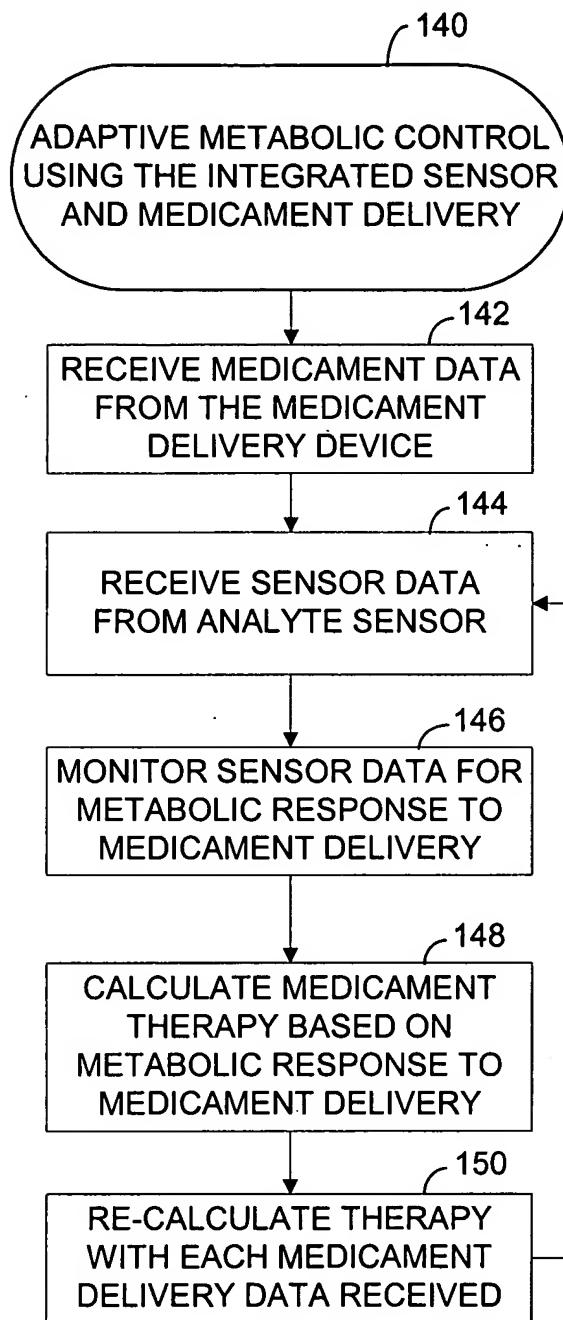


FIG. 10

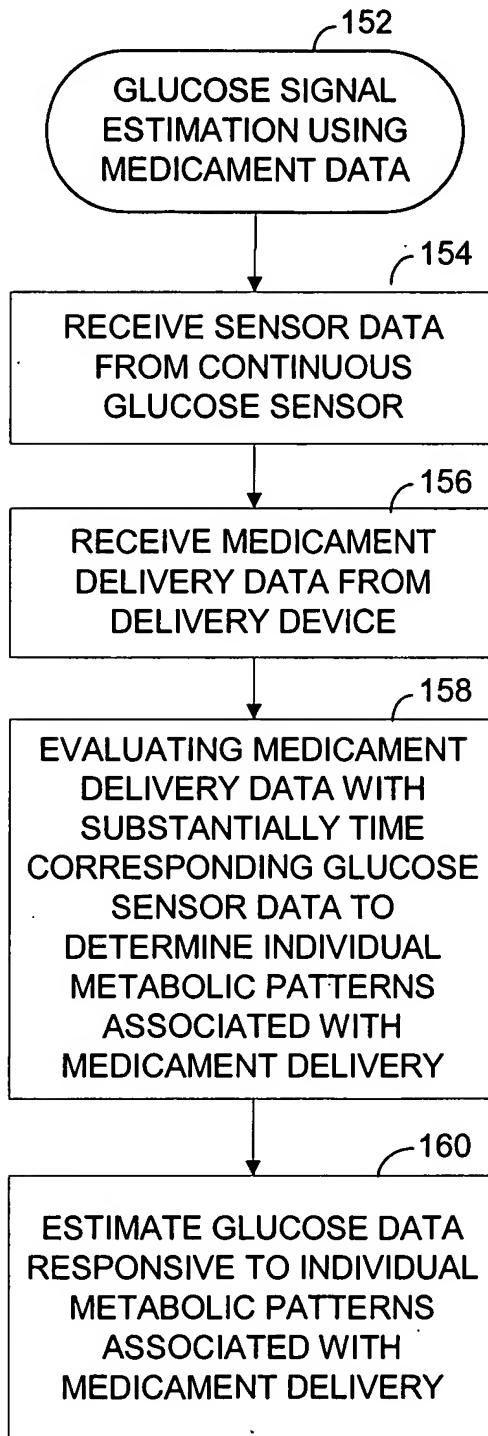


FIG. 11